



EnMAP Onboard Calibration

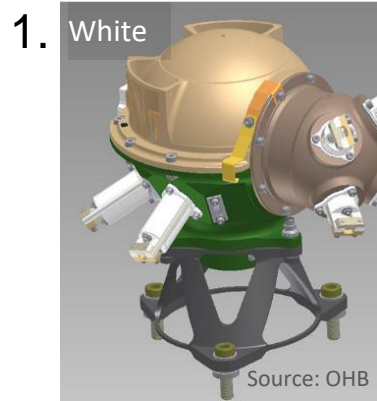


1. **OBCA-Radiometric Stability** Lamp calibration with white spectralon sphere, frequency: weekly

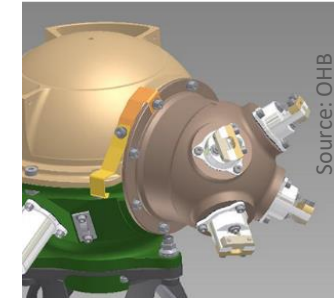


2.

2. **OBCA-Spectral** Spectral calibration with doped spectralon sphere, frequency: 2 weeks

3.

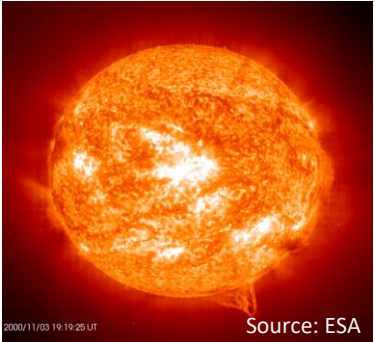

3. **Absolute Radiometric** Sun calibration with sun diffuser, frequency: monthly

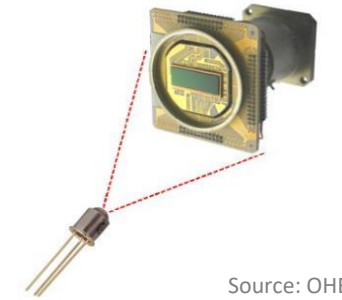

4.

4. **Linearity Calibration** with LEDs in front of focal plane, frequency: monthly

5A.



5. **A. Shutter Calibration Mechanism** Deep Space calibration, frequency: monthly

5. **B. Shutter Calibration Mechanism** dark measurement, frequency: before and after every image acquisition





5B.





Change in Calibration Measurements – April-December 2022



- OBCA-Radiometric Lamp

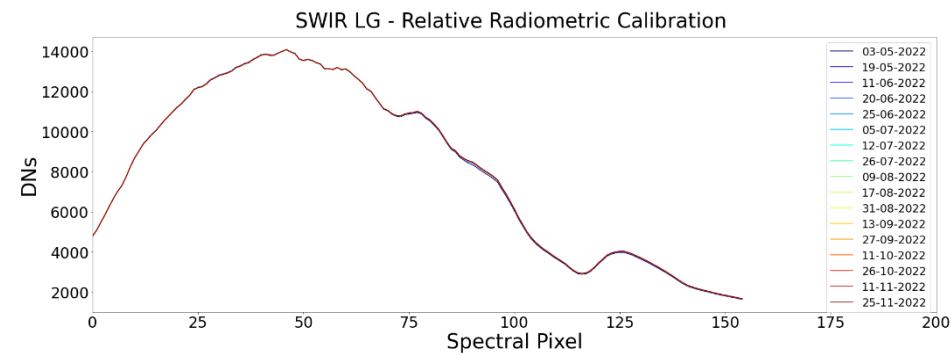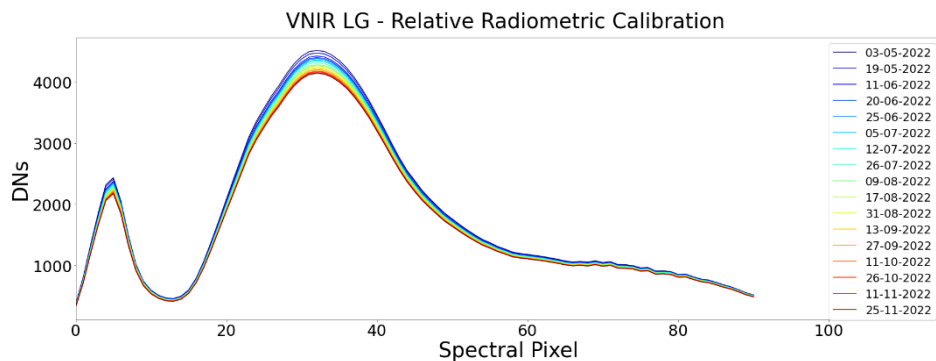

- OBCA-Spectral

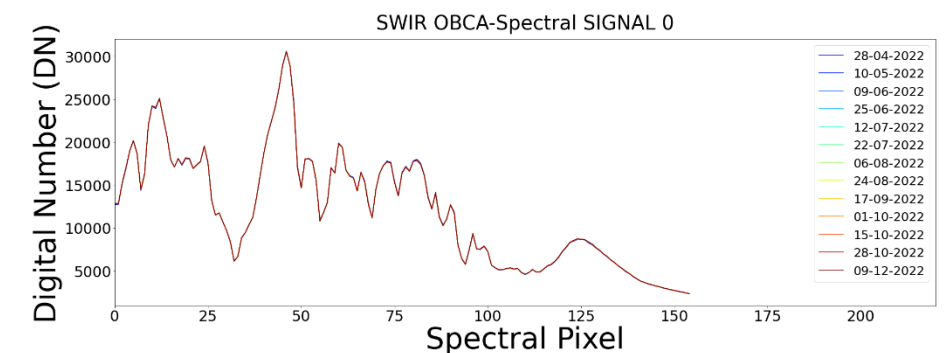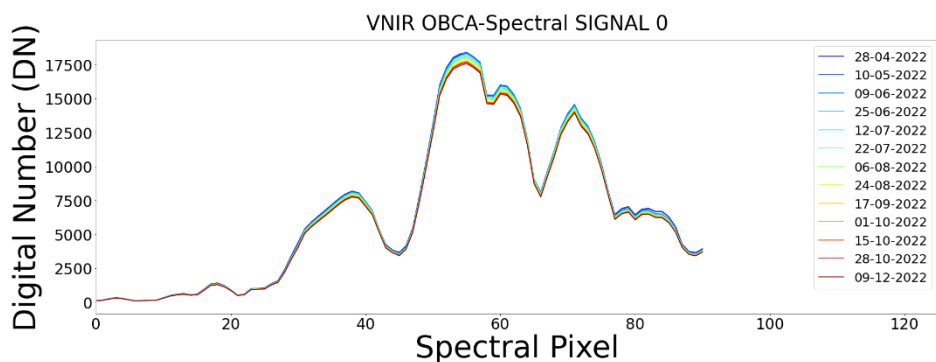


- Linearity





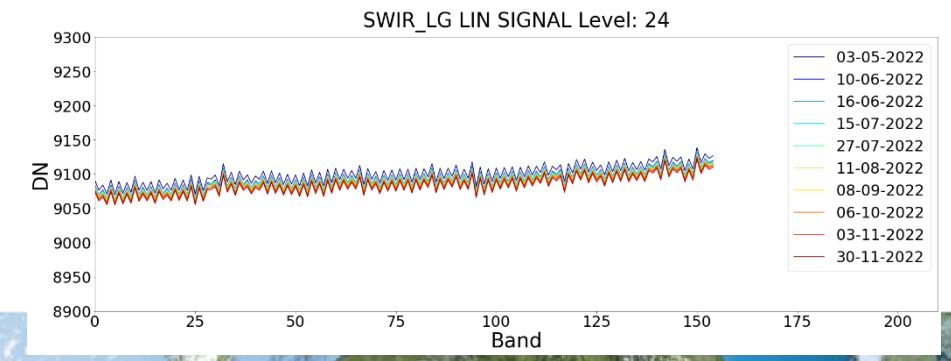
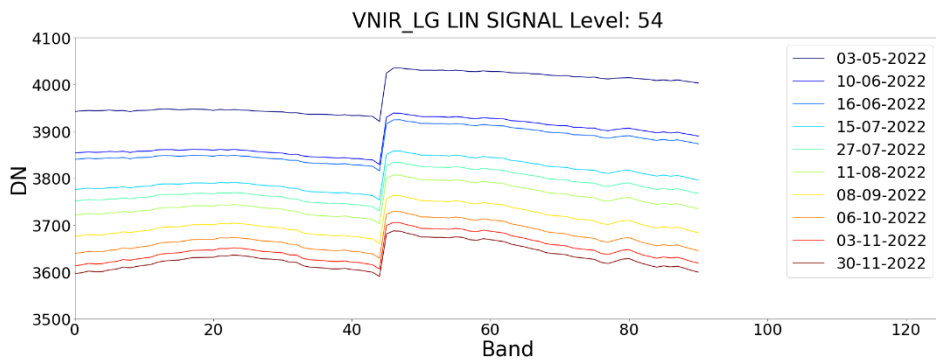


Degradation Distribution Pattern

- Degradation map from OBCA-Radiometric Lamp in VNIR HG
- Percentage change from May – November 2022

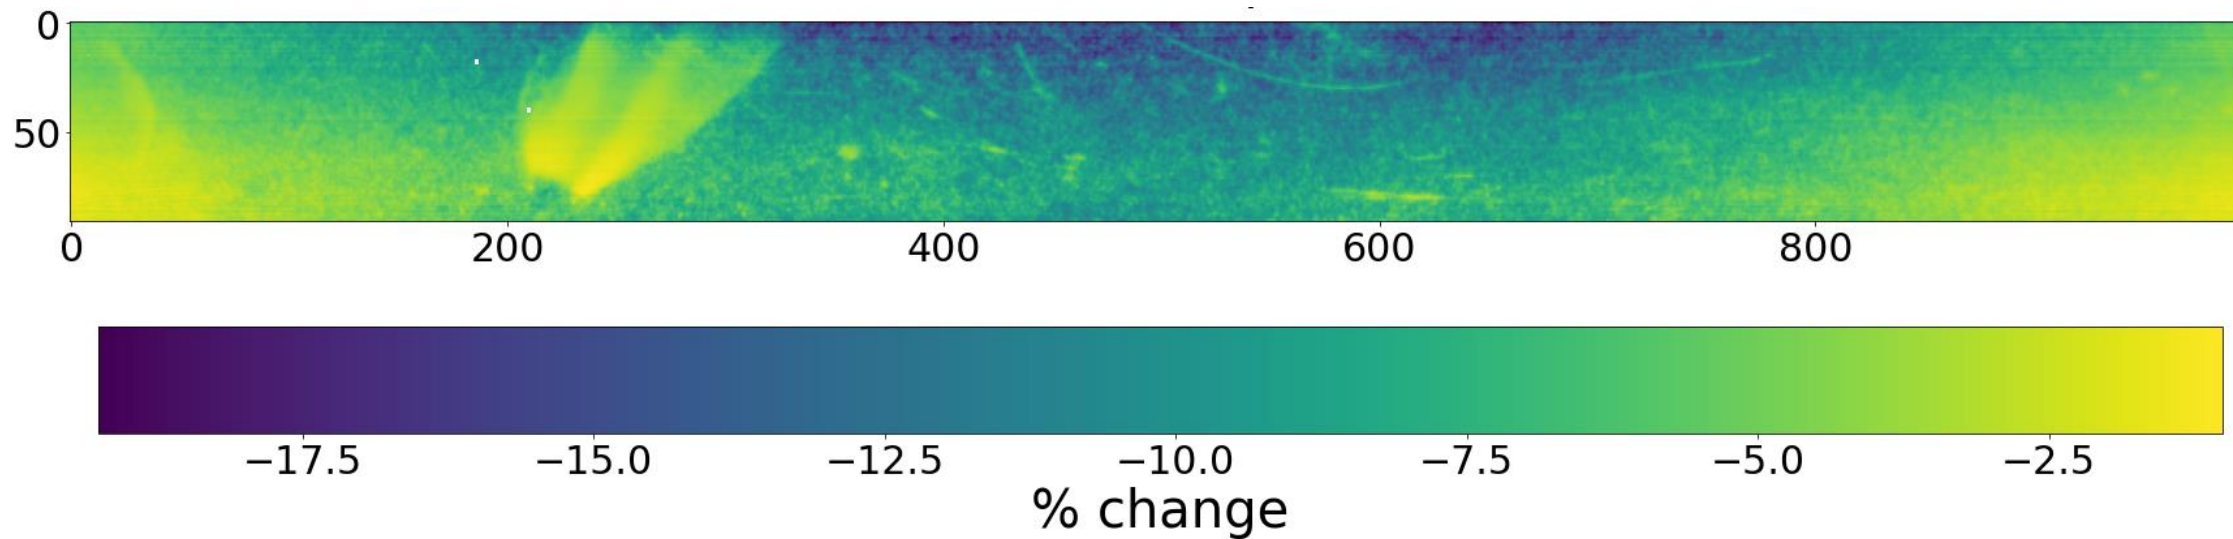

Absolute Radiometric Calibration Coefficients – April-December 2022

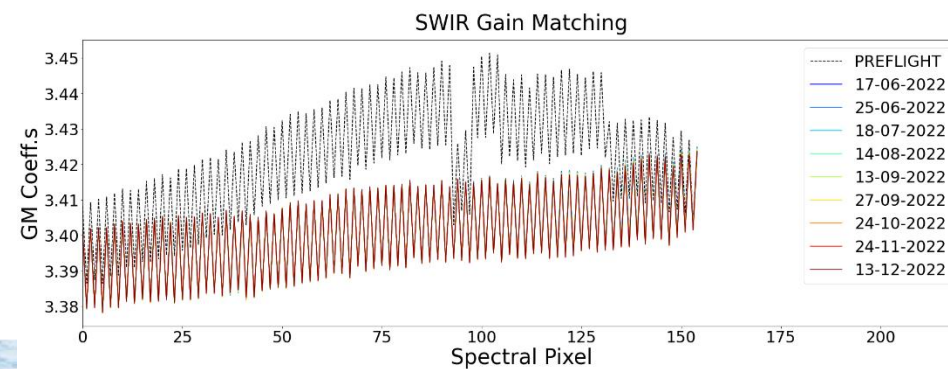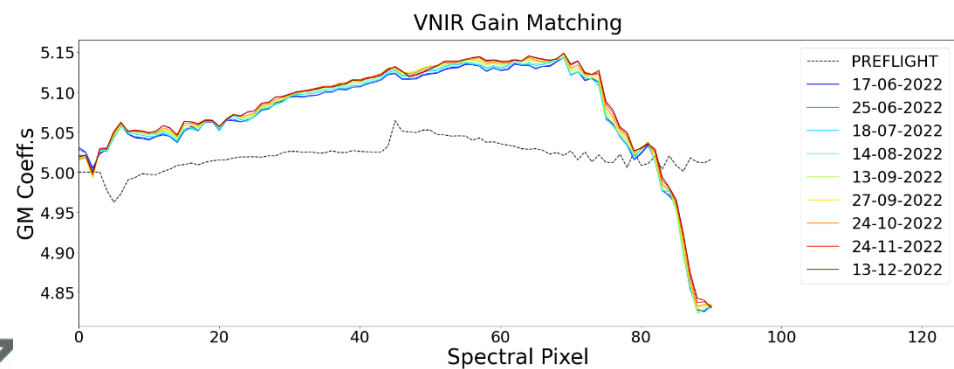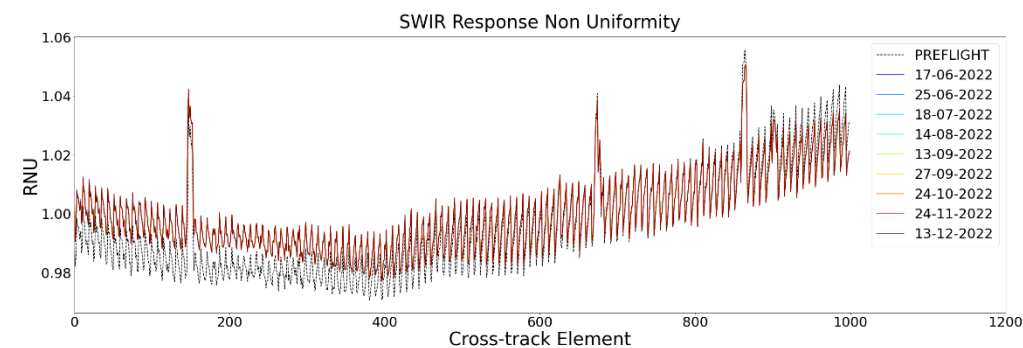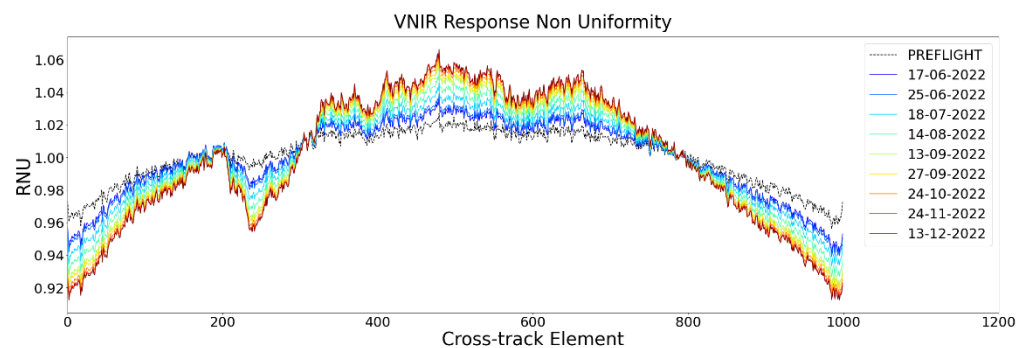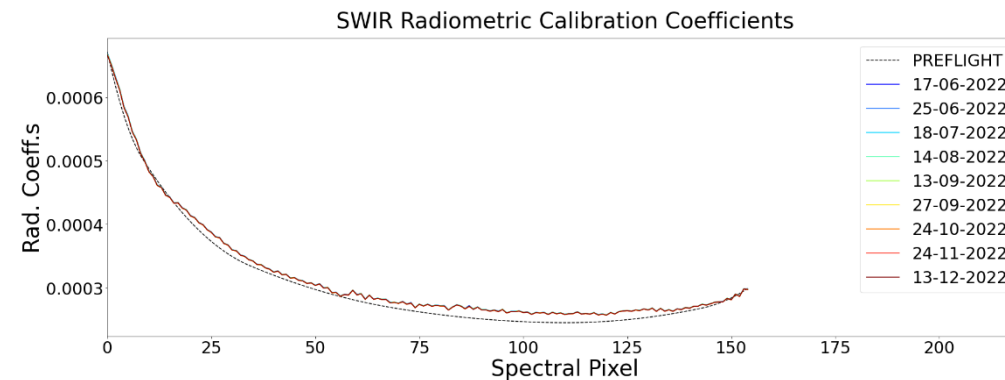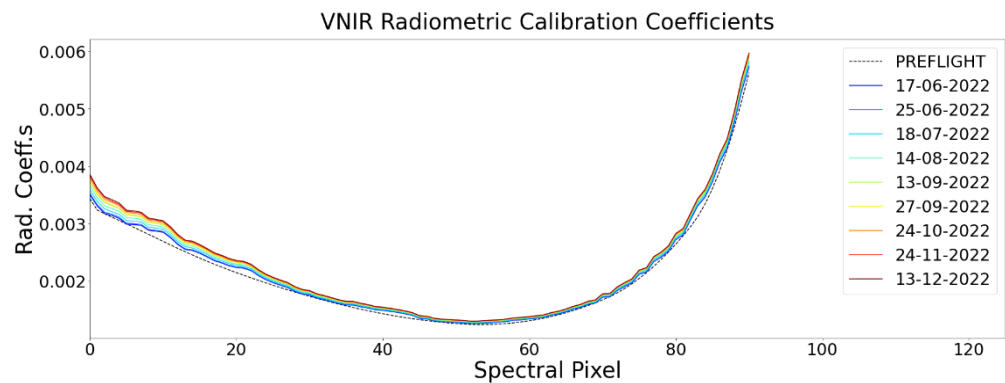


Dynamic Coefficients

Due to fast degradation in VNIR sensor, calibration tables used in L1B processing could become outdated quickly

Solution: model VNIR RNU and radiometric behaviour with „Dynamic Coefficients“ from an exponential-polynomial function

Dynamic Coefficients are used between April – December 2022 rather than coefficients in calibration tables

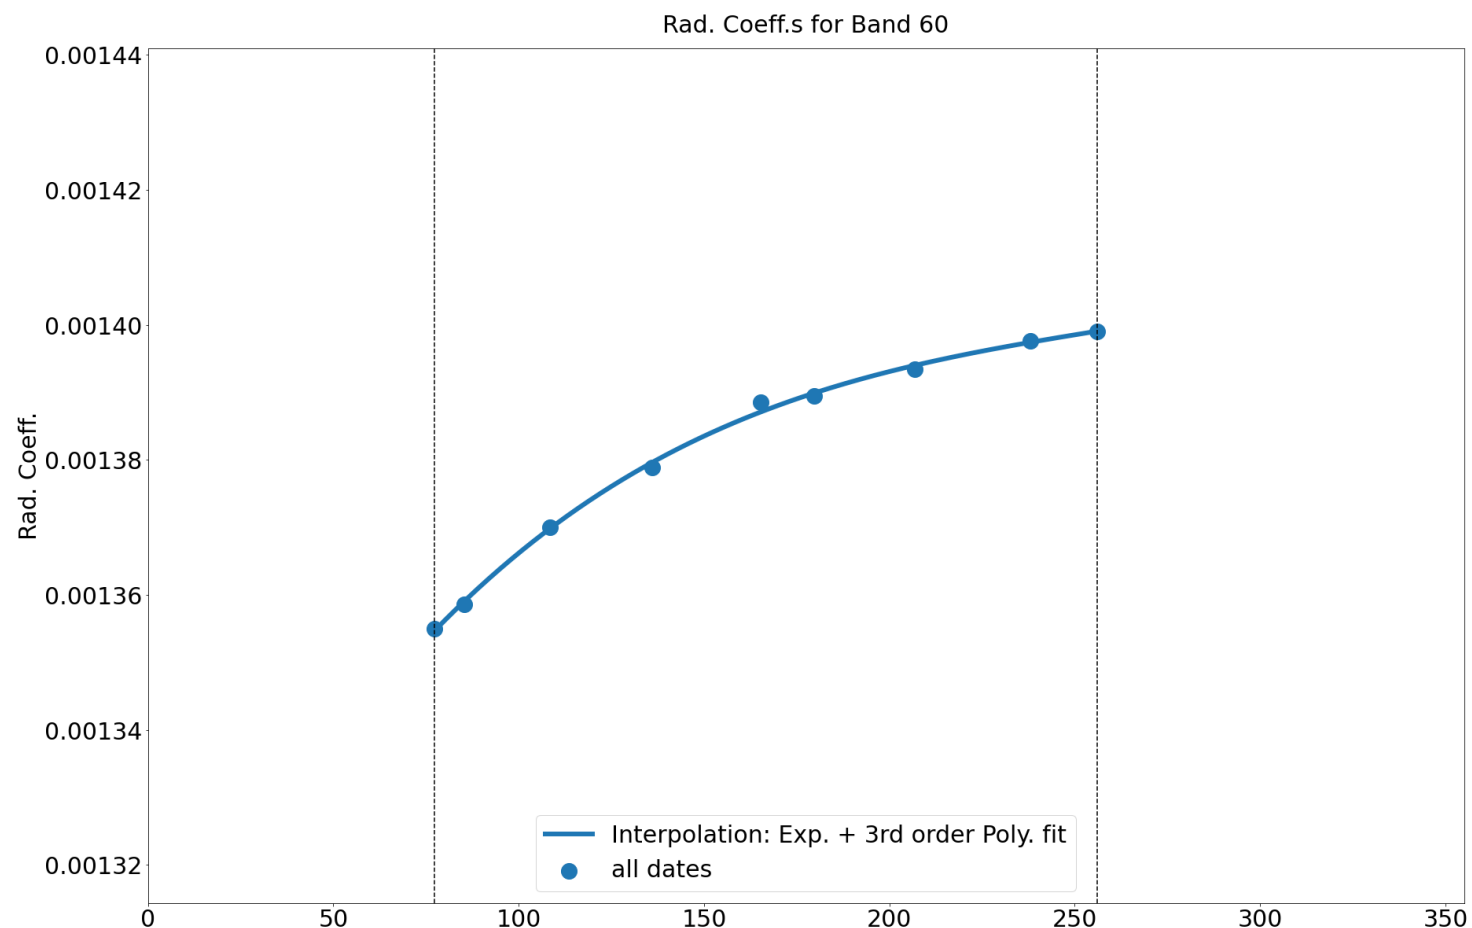



$$\text{Coefficient}^{RNU/CC} = Ae^{Bx} + Cx^3 + Dx^2 + Ex + F$$

X is days from 1st April 2022





Change in Calibration Measurements – February-July 2023



- OBCA-Radiometric Lamp

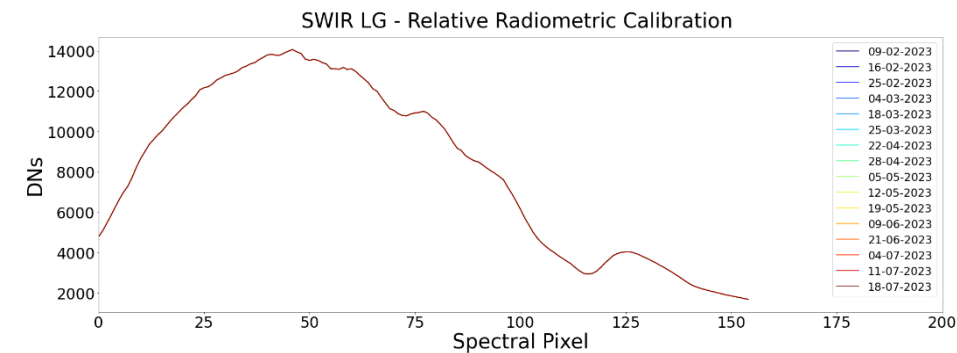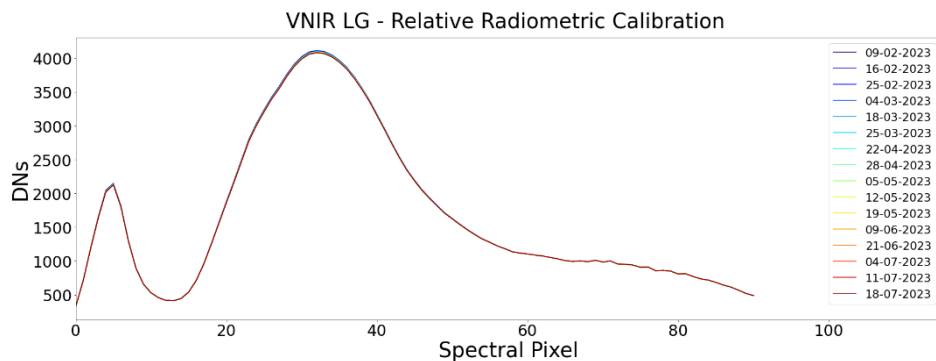

- OBCA-Spectral


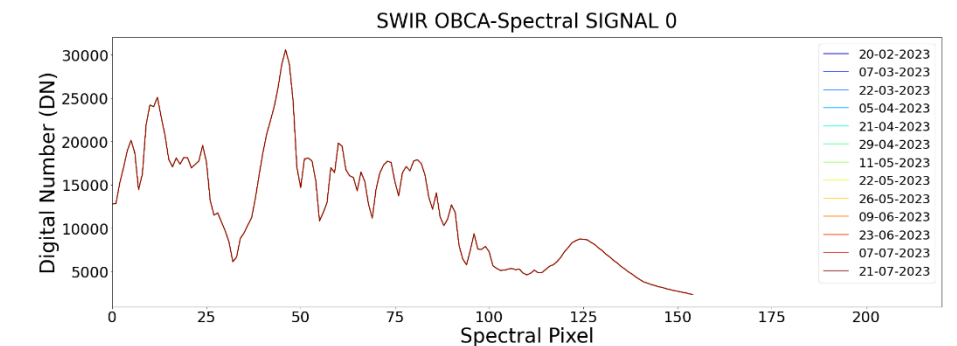
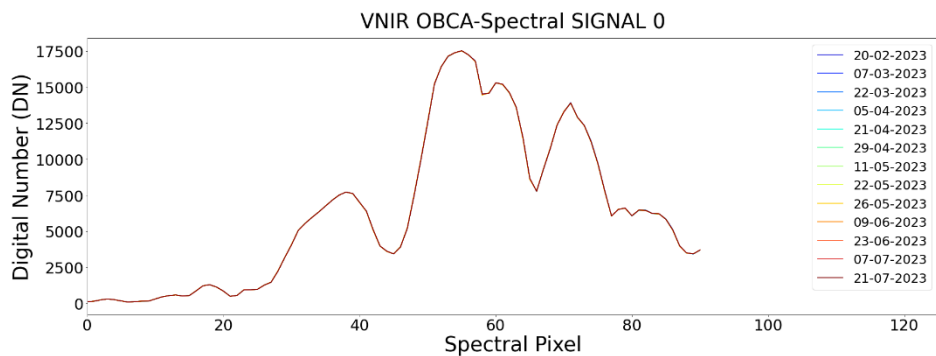


- Linearity





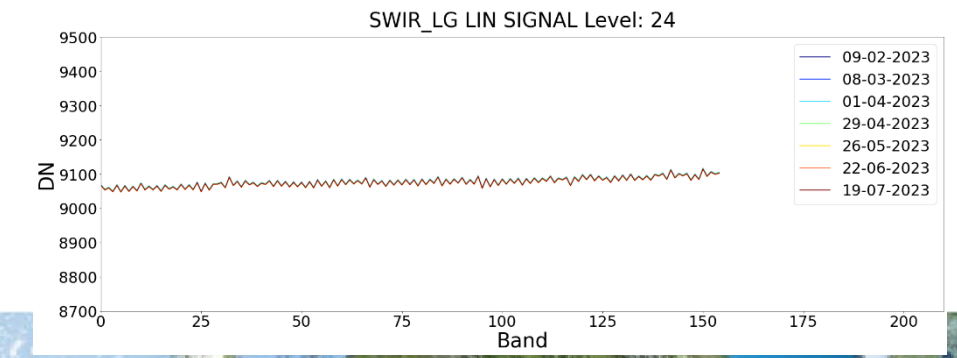
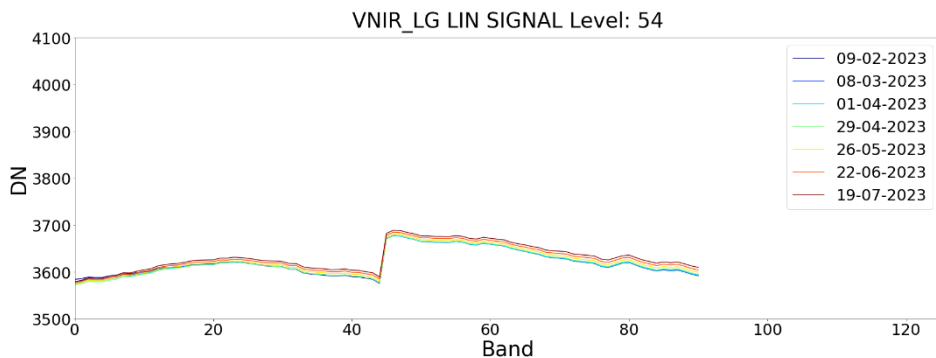


Change in Degradation per Day

- Degradation per day calculated from OBCA-Radiometric, OBCA-Spectral and Linearity measurements
- Large values during Commissioning Phase (-0.05% per day)
- Values decreasing over time
- Approximately zero degradation now (with some variability)
- Cause still unknown
- Total loss around 10%

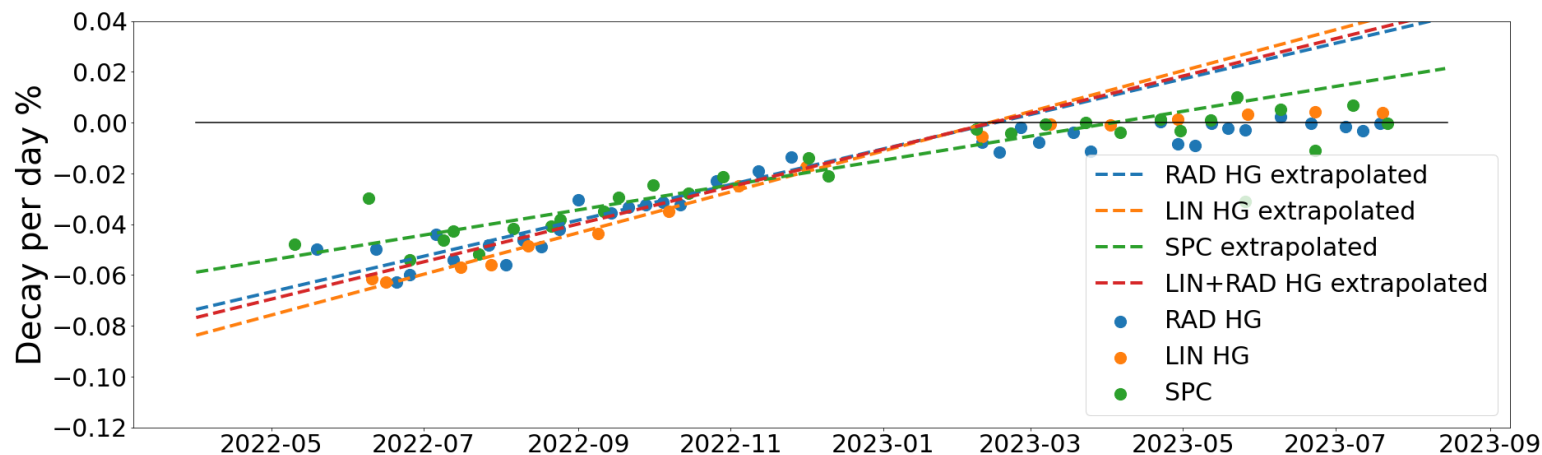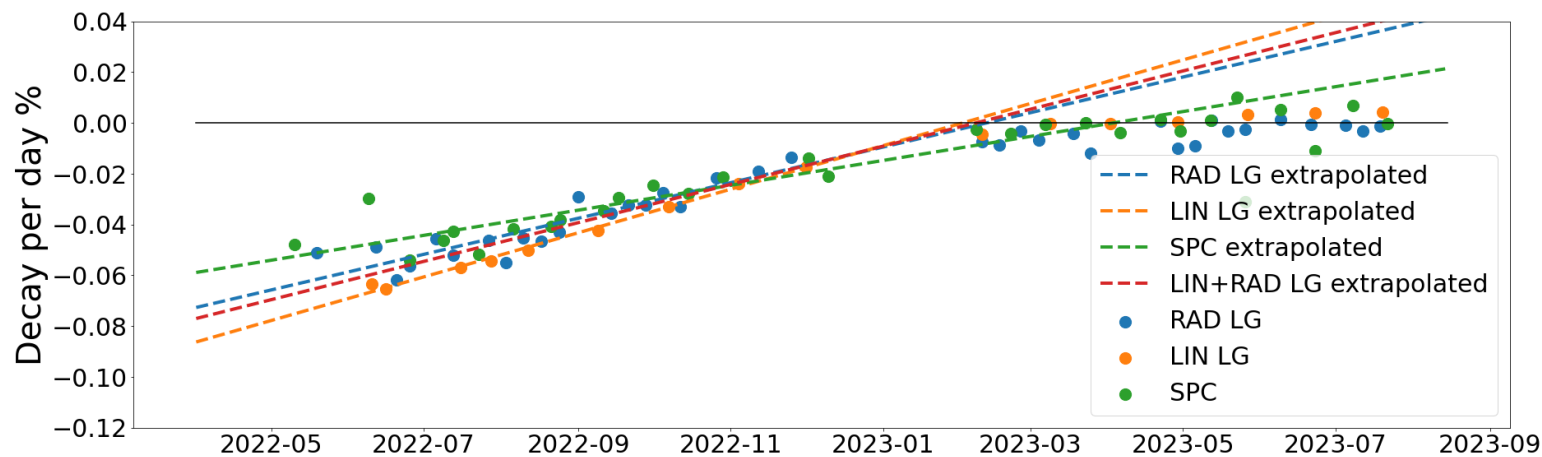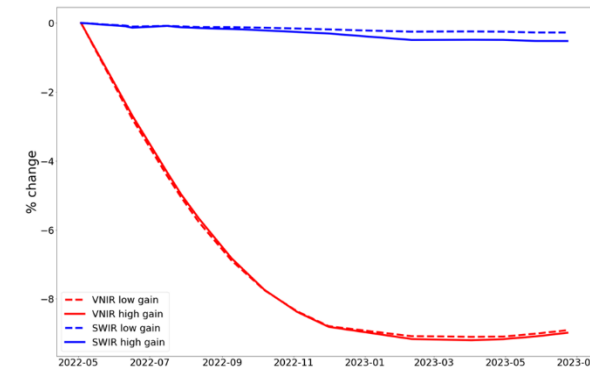


Calibration Coefficients

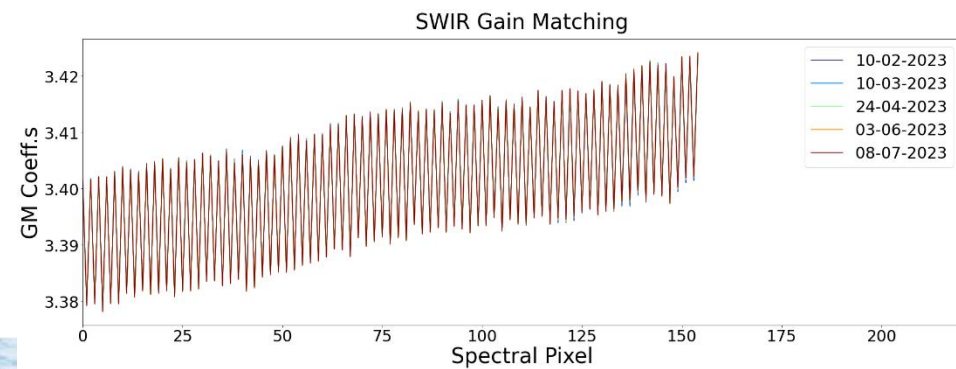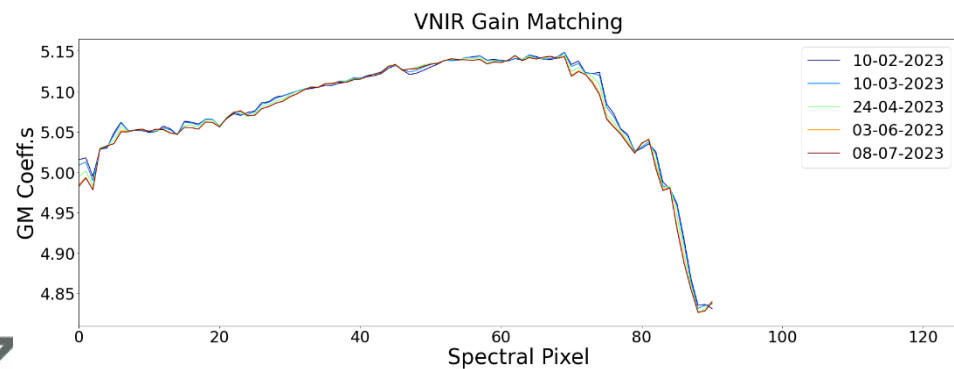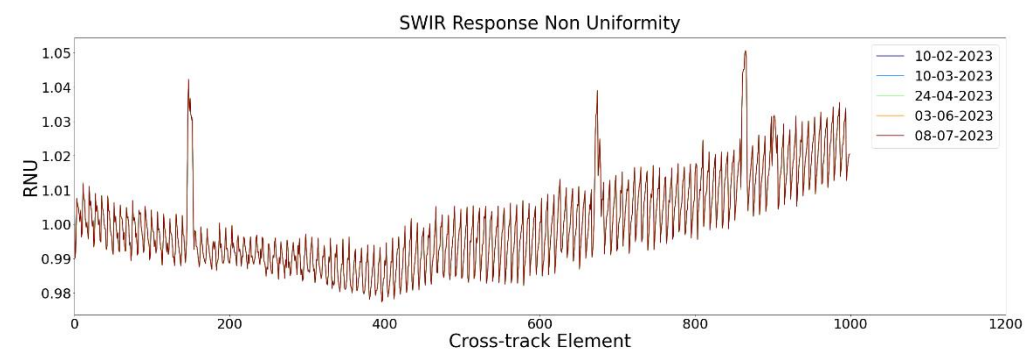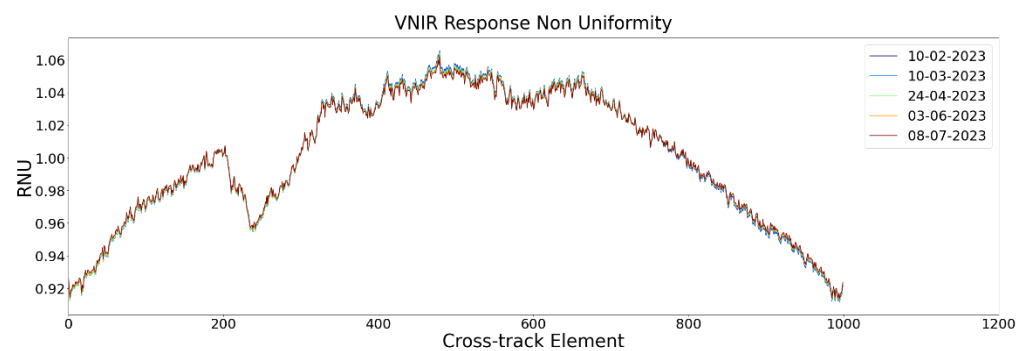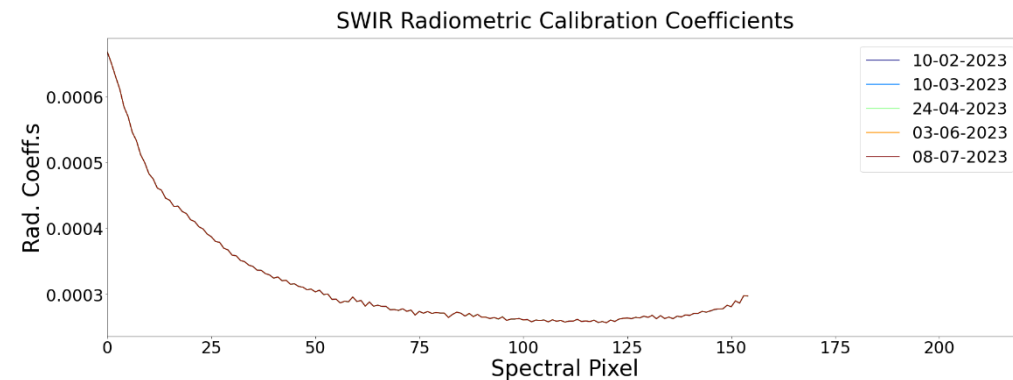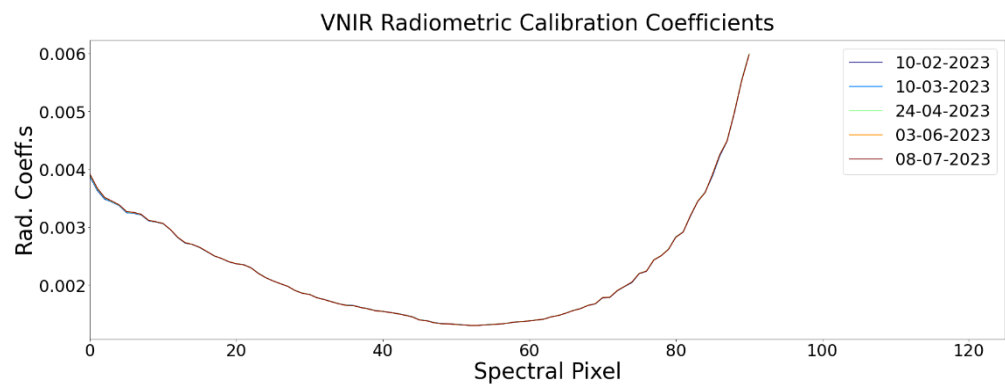


Spectral stability

VNIR OBCA Spectral change in centre wavelength

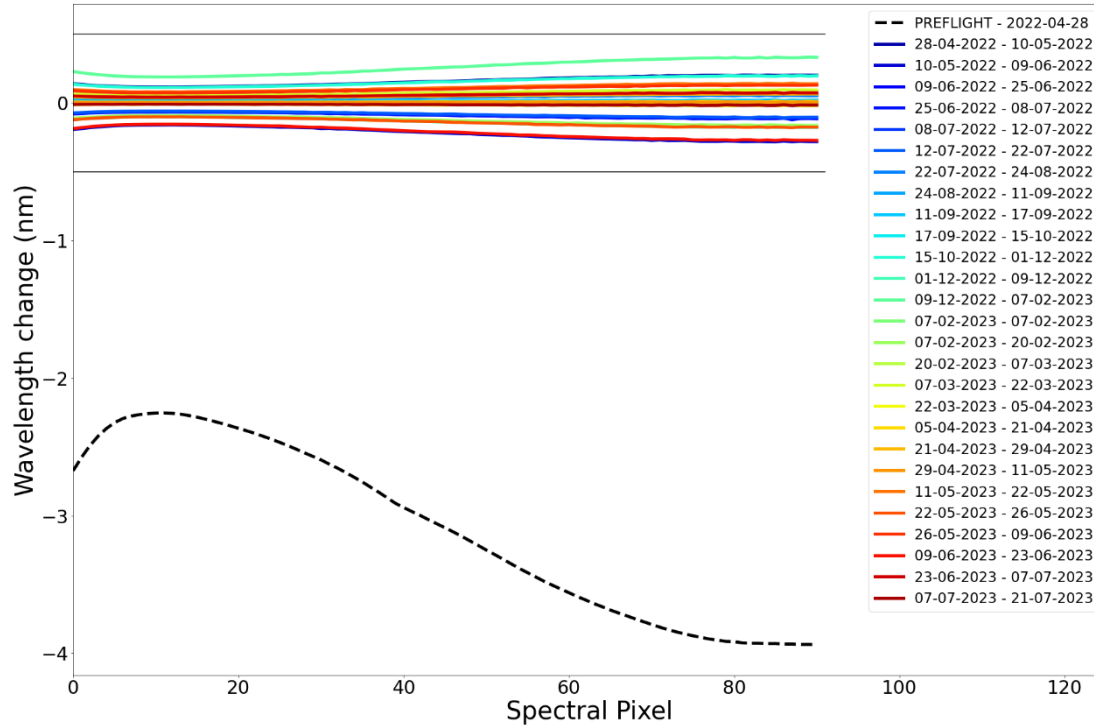

SWIR OBCA Spectral change in centre wavelength

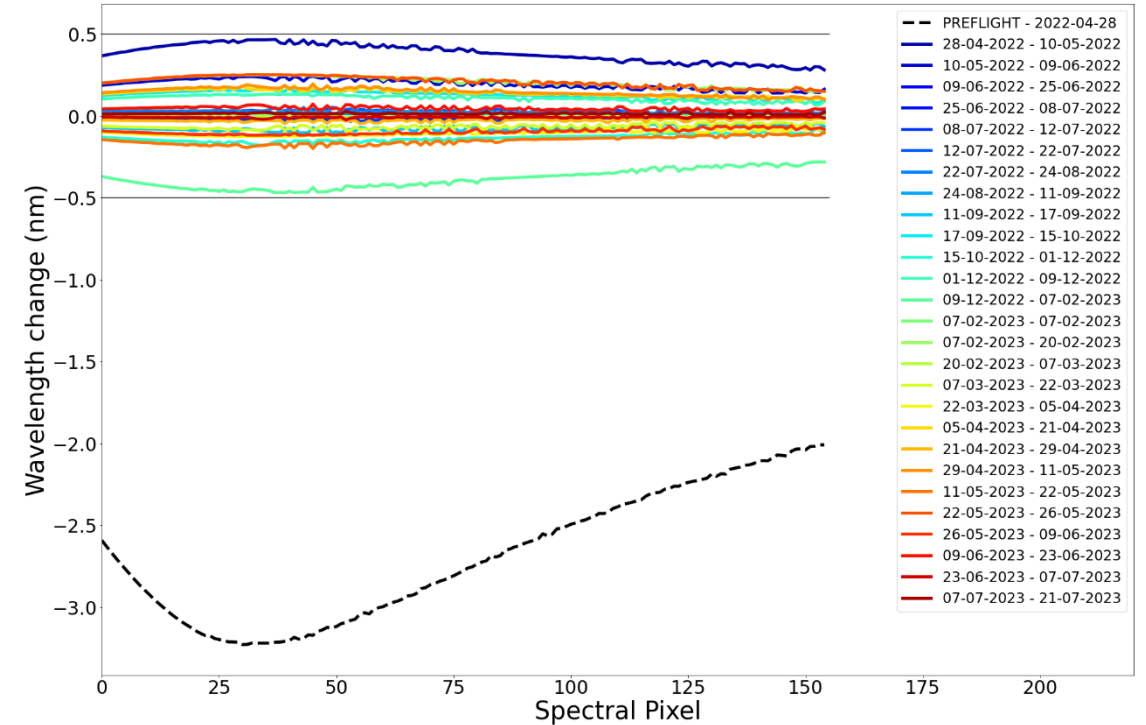

- Good spectral stability: within requirements (0.5 nm VNIR, 1.0 nm SWIR)
- 6 spectral updates during mission (4 during Commissioning, 1 after outage, 1 for SWIR band swap)



Summary

	April – December 2022	January 2023 – Present
VNIR sensor	Degradation (10%)	Stable
VNIR radiometric calibration coefficients	Changes due to degradation, dynamic coefficients used	Stable (meets 2.5% requirement between observations), calibration tables used
SWIR sensor	Stable after launch	Stable
SWIR radiometric calibration coefficients	Stable after launch (meets 2.5% requirement between observations)	Stable (meets 2.5% requirement between observations)
Dark Signal	Stable	Stable
VNIR spectral calibration	Stable after launch (meets 0.5 nm requirement)	Stable (meets 0.5 nm requirement)
SWIR spectral calibration	Stable after launch (meets 1.0 nm requirement)	Stable (meets 1.0 nm requirement)

